

**ResMed**

**AirFit™** P10

Nasal pillows mask



**reddot** award 2014  
winner

## A quieter mask to fit your patients

ResMed's AirFit™ P10 nasal pillows mask is part of ResMed's AirFit range—the right fit for your patients. This is our quietest mask yet, offering the reliability and performance of the Swift™ FX in a design that's 50% quieter and around 50% lighter.

### Quieter

QuietAir™ woven-mesh vent is whisper quiet at just 21.4 dBA<sup>3</sup>, for minimal patient and partner disturbance.

### Lighter

It's almost 50% lighter than our most popular pillows mask and designed to provide a comfortable night's sleep.

### Easy to fit

QuickFit™ elastic headgear automatically adjusts to each patient's head. It can be fitted in under 30 seconds.<sup>2</sup>

# More than 40 minutes of extra sleep ...

In a recent ResMed study<sup>1</sup> with 21 current CPAP users from Australia, we found that on average, patients slept more than 40 minutes longer per night using the ResMed AirFit P10 compared to the Swift FX mask.

For more information on the study see: [ResMed.com/AirFitP10](https://www.resmed.com/AirFitP10)  
Whitepaper 'Assessment of a new nasal pillows mask in patients receiving CPAP'.



## AirFit P10 features and benefits

**Dual-wall technology**  
with trampoline action seals on contact, dispersing air gently to the nose.


**Key-clip nasal pillows**  
offer effortless assembly, with colour coding for easy sizing and left/right orientation to ensure patients fit the mask properly.

**Innovative flexi-tube**  
is ultra-light and flexible yet highly durable, offering patients freedom of movement without compromising seal.

**QuietAir™ woven-mesh venting**  
quietly diffuses exhaled air and is barely noticeable to patients and their bed partners. It's ResMed's quietest mask at just 21.4 dBA.<sup>3</sup>

**QuickFit™ elastic headgear**  
with unique split-strap design provides stability and adjustability with minimal facial contact.

**The AirFit P10 for Her**  
is designed especially for women, offering a smaller size for female facial contours, finished in stylish tones and highlights.

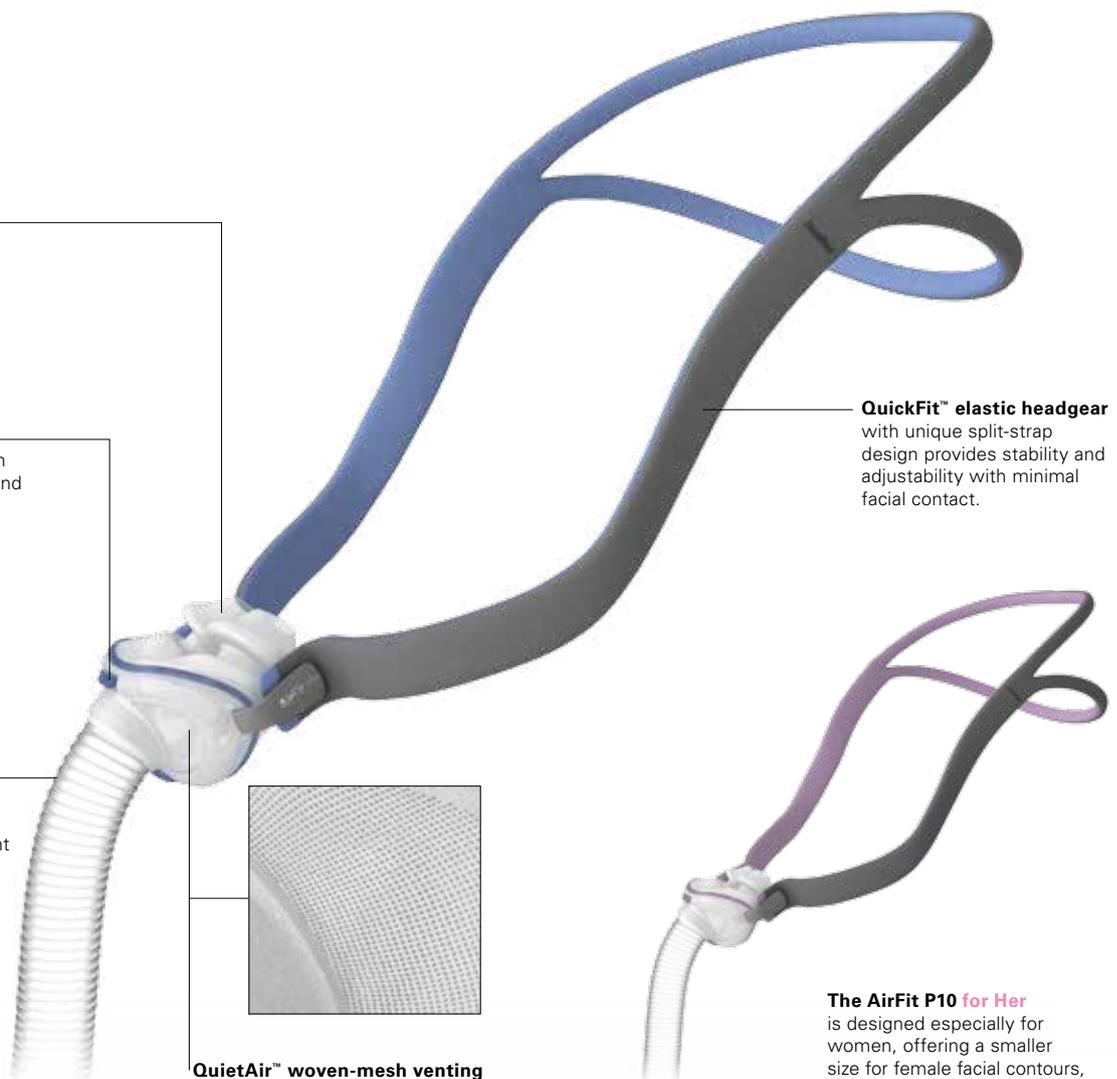

# AirFit P10 components




QuickFit elastic headgear  
**62935** Standard size

QuickFit for Her elastic headgear  
**62936** Small size




Frame  
**62938**

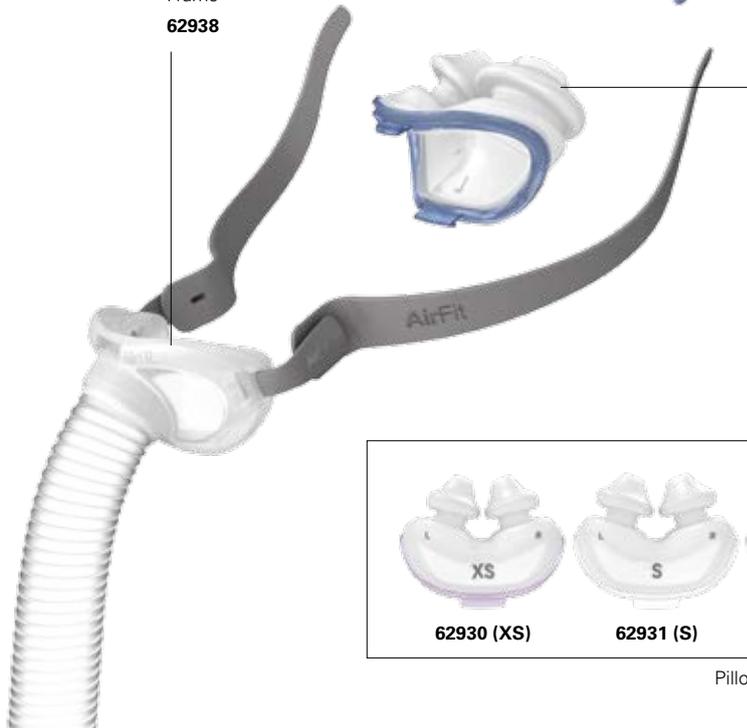

## 3-part simplicity

makes the AirFit P10 mask around 50% lighter than the leading nasal pillows mask.

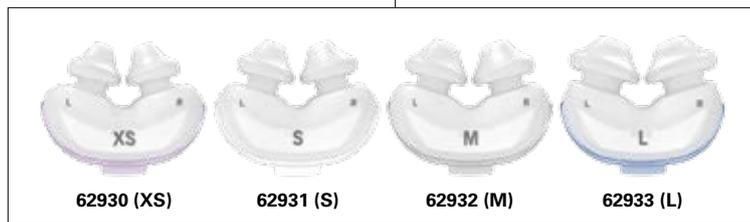

**62930 (XS)**

**62931 (S)**

**62932 (M)**

**62933 (L)**

Pillows

- XS** Extra Small
- S** Small
- M** Medium
- L** Large

## Product codes

|  | Europe 1     | Europe 2     | Europe 3     |
|--|--------------|--------------|--------------|
| AirFit P10 - complete system*          | <b>62901</b> | <b>62902</b> | <b>62903</b> |
| AirFit P10 for Her - complete system** | <b>62911</b> | <b>62912</b> | <b>62913</b> |

**Note:** For more details, refer to the AirFit P10 User Guide.

\* S, M and L pillows are included with the mask and standard size headgear (blue).

\*\* XS, S and M pillows are included with the mask and small size headgear (pink).


**Europe 1:** English (UK), French, German and Italian (Switzerland)

**Europe 2:** English, Danish, Estonian, Finnish, Norwegian and Swedish

**Europe 3:** English, Czech, Dutch (Belgium), French (Belgium), German (Belgium), Greek, Hungarian, Italian, Polish, LMSXS Portuguese, Russian, Slovak, Spanish and Turkish

**AirFit™ P10**

Nasal pillows mask

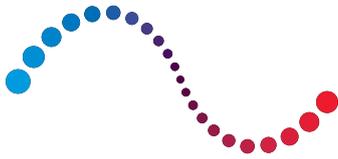

# ResMed

## AirFit™ P10

Nasal pillows mask

### Fitting guide for AirFit P10




- Hold the pillows at your nose, ensuring that the pillow size indicator is on the bottom and you can see the left (L) and right (R) orientation indicators.



- Stretch the lower strap around the back of your head.
- The top strap should sit comfortably on top of your head.



- Pull the headgear over your head by holding the lower strap.

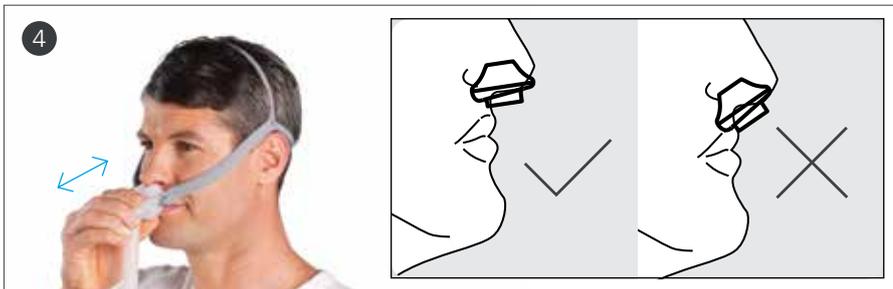

- Move the mask away from your face, and then place it back again.
- Ensure the nasal pillows fit securely into your nostrils with both pillows positioned upright.



- Finally, connect the end of the mask's tube into your device's air tubing.
- Turn on your device — your mask is now ready to use. A light breeze should be felt through the vent.



- If adjustment is needed, spread the upper and lower straps apart to loosen, or draw them closer together to tighten.

**Note:** For complete user instructions, refer to the AirFit P10 User Guide.

1 ResMed Study FECS3. ResMed data (pressure, leak, average daily usage, AHI) collected from a sample size of 21 participants.

2 ResMed Study FECS3. 90% of participants fitted the mask comfortably in less than 30 seconds.

3 Declared dual numbered noise emission values (with uncertainty 3dB(A)) in accordance with ISO 4871.



**ResMed Ltd**  
1 Elizabeth Macarthur Drive,  
Bella Vista, NSW 2153 Australia

**DISTRIBUTED BY**  
**EC REP** ResMed (UK) Ltd, 96 Jubilee Avenue,  
Milton Park, Abingdon, Oxfordshire, OX14 4RW UK

AirFit, QuickFit, QuietAir and Swift are trademarks of ResMed Ltd. Swift is registered in the U.S. Patent and Trademark Office. Product availability may vary across regions. Specifications may change without notice. © 2014 ResMed Ltd. 1016674/3 2014-03

